


Peak Analysis

Injection Details			
Injection Name:	1,M-2-N3		Run Time (min): 15.53
Vial Number:	76		Injection Volume: 1.00
Injection Type:	Calibration Standard		
Calibration Level:			
Instrument Method:	50 hold 2 min 20 per 150 hold 30 per 280 hold 3 min		
Processing Method:	Qualitative		Dilution Factor: 1.0000
Injection Date/Time:	24/Nov/22 15:44		Sample Weight: 1.0000

Chromatogram

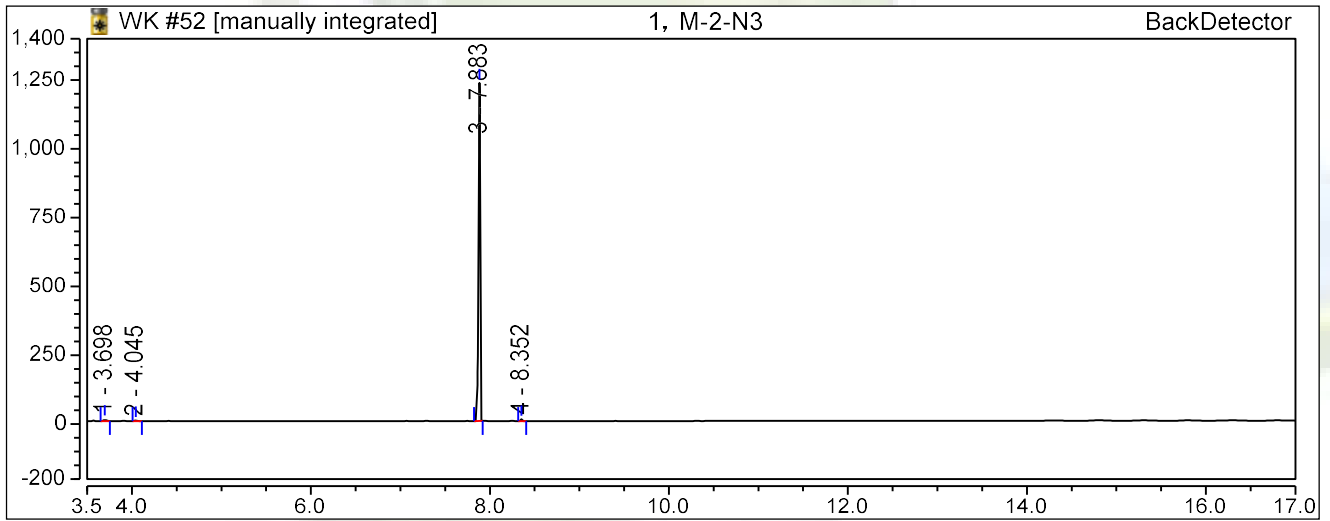

No.	Peak Name	Retention Time min	Area pA*min	Height pA	Relative Area %	Relative Height %
1		3.698	0.199	8	0.72	0.62
2		4.045	0.051	2	0.19	0.18
3		7.883	27.090	1,229	98.64	97.0
4		8.352	0.124	6	0.45	0.51
Total:			27	1,246	100.00	100.00

