


## Peak Analysis

Injection Details					
Injection Name:	m-4-sh			Run Time (min):	10.67
Vial Number:	101			Injection Volume:	3.00
Injection Type:	Unknown				
Calibration Level:					
Instrument Method:	80 hold 2 min 30 per 280 hold 2 min				
Processing Method:	Qualitative			Dilution Factor:	1.0000
Injection Date/Time:	02/Oct/23 14:47			Sample Weight:	1.0000

## Chromatogram

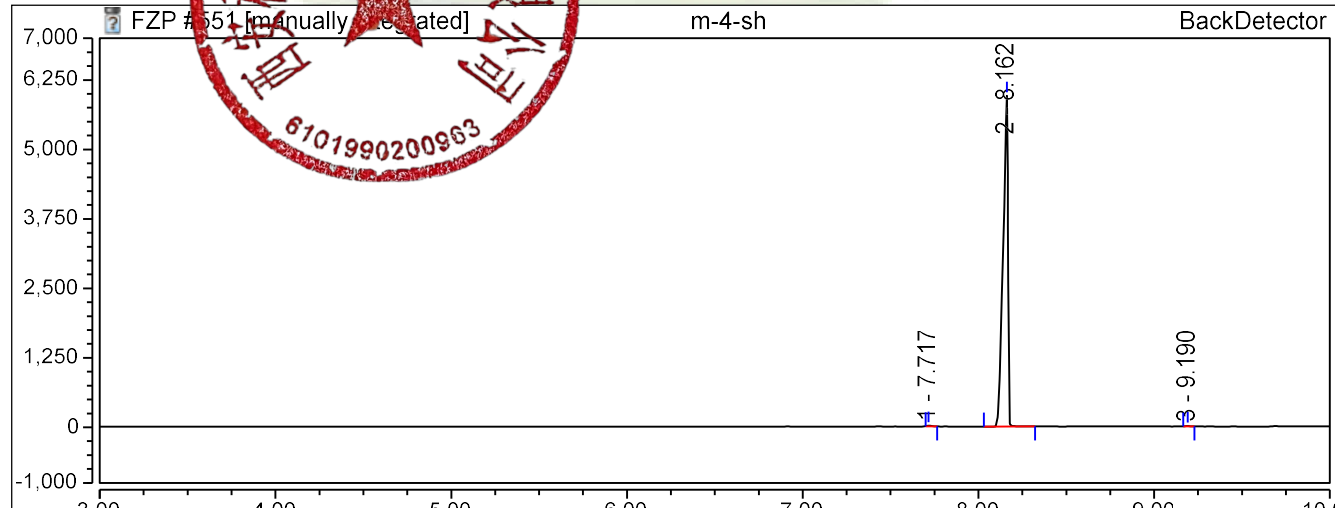

No.	Peak Name	Retention Time min	Area pA*min	Height pA	Relative Area %	Relative Height %
1		7.717	0.313	10	0.16	0.17
2		8.162	190.757	5,951	99.70	99.65
3		9.190	0.266	10	0.14	0.17
Total:			191	5,972	100.00	100.00

### Mass Spectrum

Spectral plot could not be created.  
No spectra selected.