


Peak Analysis

Injection Details					
Injection Name:	m-5-SH-?800G			Run Time (min):	10.67
Vial Number:	61			Injection Volume:	3.00
Injection Type:	Unknown				
Calibration Level:					
Instrument Method:	80 hold 2 min 30 per 280 hold 2 min				
Processing Method:	Qualitative			Dilution Factor:	1.0000
Injection Date/Time:	27/Oct/23 14:54			Sample Weight:	1.0000

Chromatogram

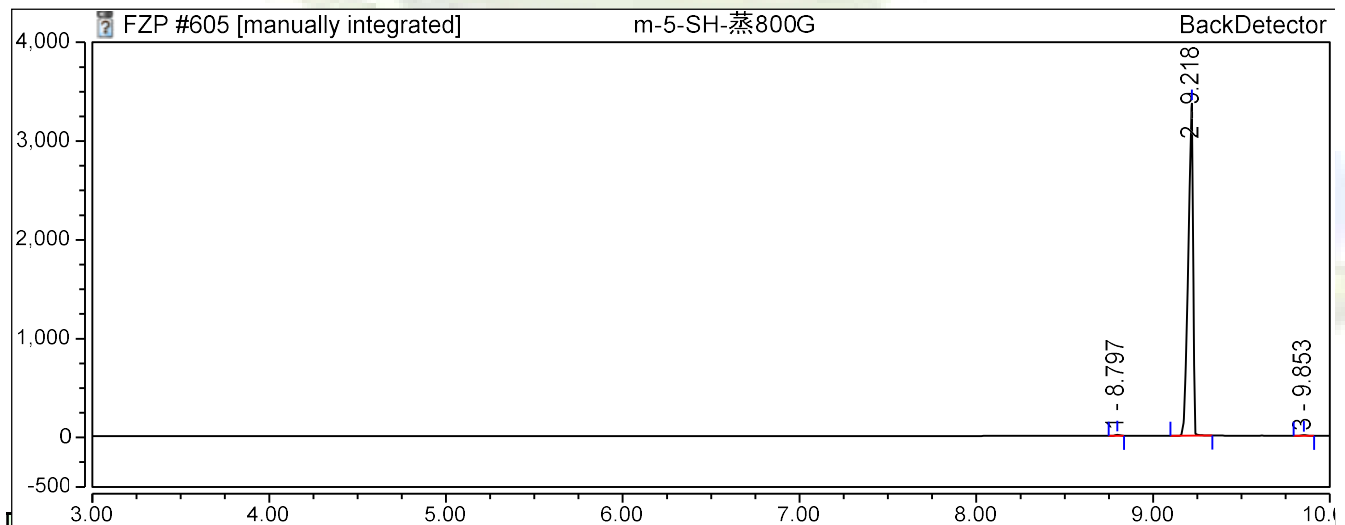

No.	Peak Name	Retention Time min	Area pA*min	Height pA	Relative Area %	Relative Height %
1		8.797	0.251	9	0.23	0.28
2		9.218	108.074	3,363	99.55	99.51
3		9.853	0.234	7	0.22	0.21
Total:			109	3,379	100.00	100.00

Mass Spectrum

Spectral plot could not be created.
No spectra selected.