


## Peak Analysis

Injection Details					
Injection Name:	1.28 MPEG6-OH			Run Time (min):	16.50
Vial Number:	14			Injection Volume:	1.00
Injection Type:	Calibration Standard				
Calibration Level:					
Instrument Method:	100 hold 2 min 25 per 280 hold 6 min				
Processing Method:	mjj-0426			Dilution Factor:	1.0000
Injection Date/Time:	28/Jan/24 10:42			Sample Weight:	1.0000

## Chromatogram

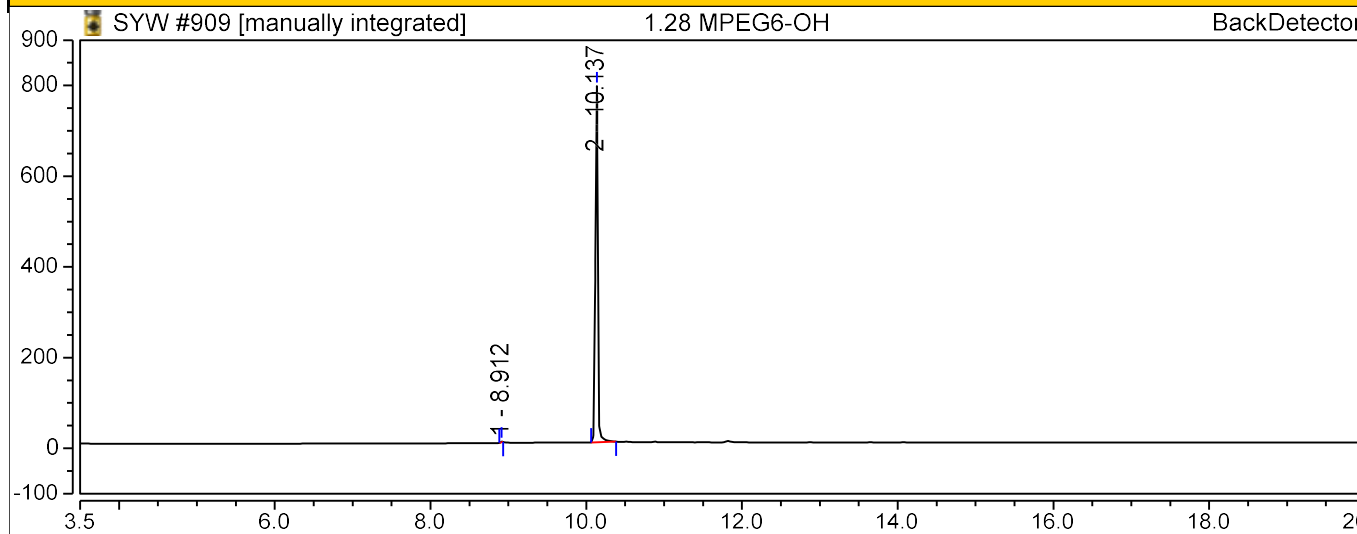

No.	Peak Name	Retention Time min	Area pA*min	Height pA	Relative Area %	Relative Height
1		8.912	0.056	2	0.20	0.28
2		10.137	28.464	785	99.80	99.72
Total:			29	787	100.00	100.00

