


## Peak Analysis

Injection Details					
Injection Name:	11.15 MPEG5-OH???(100g)-DCM?			Run Time (min):	16.50
Vial Number:	21			Injection Volume:	1.00
Injection Type:	Calibration Standard				
Calibration Level:					
Instrument Method:	100 hold 2 min 25 per 280 hold 6 min				
Processing Method:	mjj-0426			Dilution Factor:	1.0000
Injection Date/Time:	15/Nov/23 15:44			Sample Weight:	1.0000

## Chromatogram

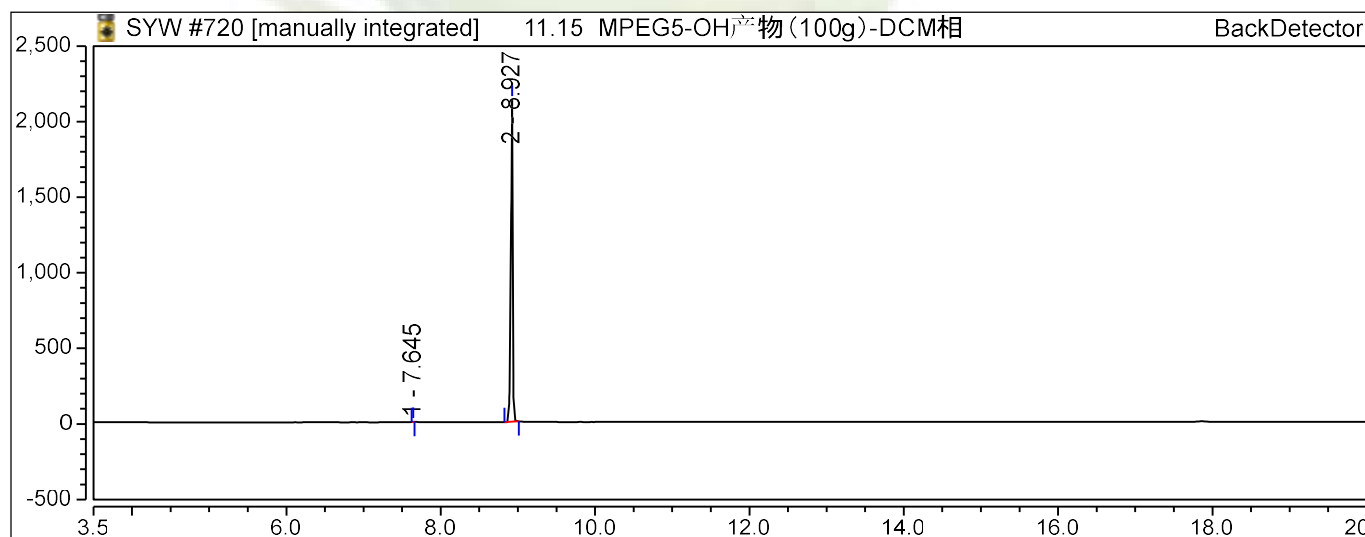

No.	Peak Name	Retention Time min	Area pA*min	Height pA	Relative Area %	Relative Height
1		7.645	0.041	2	0.06	0.08
2		8.927	64.371	2,129	99.94	99.92
Total:			64	2,131	100.00	100.00

