


Peak Analysis

Injection Details					
Injection Name:	M-3-N3-320G			Run Time (min):	10.67
Vial Number:	125			Injection Volume:	1.00
Injection Type:	Unknown				
Calibration Level:					
Instrument Method:	80 hold 2 min 30 per 280 hold 2 min				
Processing Method:	Qualitative			Dilution Factor:	1.0000
Injection Date/Time:	12/Jan/24 14:30			Sample Weight:	1.0000

Chromatogram

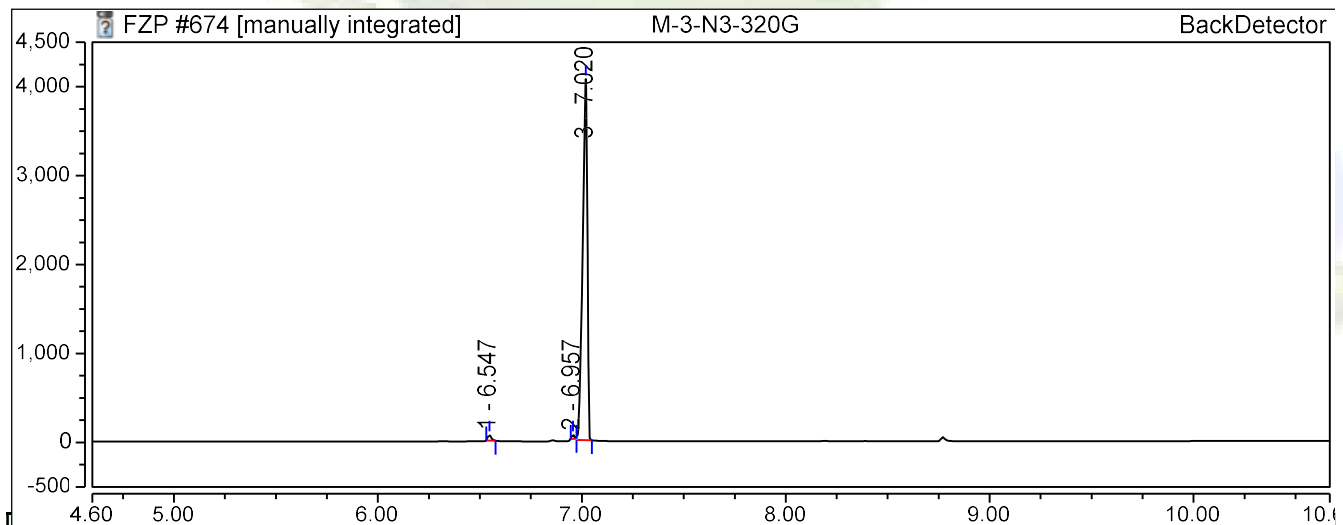

No.	Peak Name	Retention Time min	Area pA*min	Height pA	Relative Area %	Relative Height %
1		6.547	1.217	64	1.11	1.53
2		6.957	0.696	46	0.64	1.10
3		7.020	107.507	4,062	98.25	97.38
Total:			109	4,171	100.00	100.00

Mass Spectrum

Spectral plot could not be created.
No spectra selected.

