


### Peak Analysis

Injection Details					
Injection Name:	12.16 MPEG7-OH-1			Run Time (min):	16.50
Vial Number:	71			Injection Volume:	1.00
Injection Type:	Calibration Standard				
Calibration Level:					
Instrument Method:	100 hold 2 min 25 per 280 hold 6 min				
Processing Method:	mjj-0426			Dilution Factor:	1.0000
Injection Date/Time:	16/Dec/23 21:07			Sample Weight:	1.0000

### Chromatogram

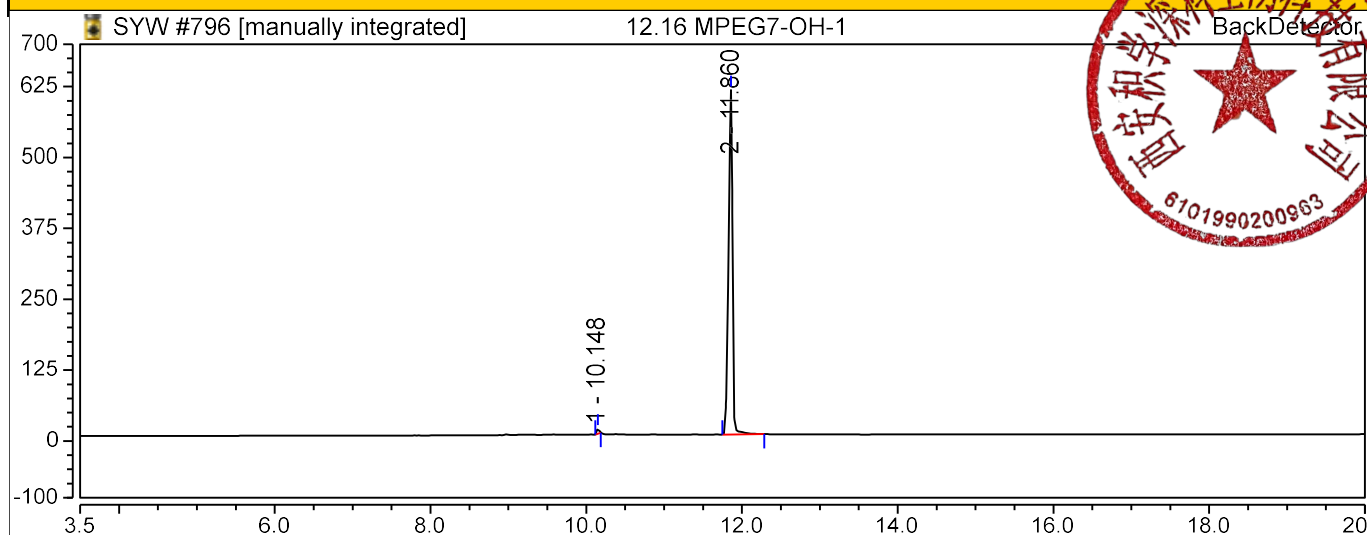

No.	Peak Name	Retention Time min	Area pA*min	Height pA	Relative Area %	Relative Height %
1		10.148	0.305	9	0.85	1.50
2		11.860	35.639	607	99.15	98.50
Total:			36	617	100.00	100.00