


Peak Analysis

Injection Details					
Injection Name:	12.12 MPEG8-OH			Run Time (min):	16.50
Vial Number:	26			Injection Volume:	1.00
Injection Type:	Calibration Standard				
Calibration Level:					
Instrument Method:	100 hold 2 min 25 per 280 hold 6 min				
Processing Method:	mjj-0426			Dilution Factor:	1.0000
Injection Date/Time:	13/Dec/23 10:20			Sample Weight:	1.0000

Chromatogram

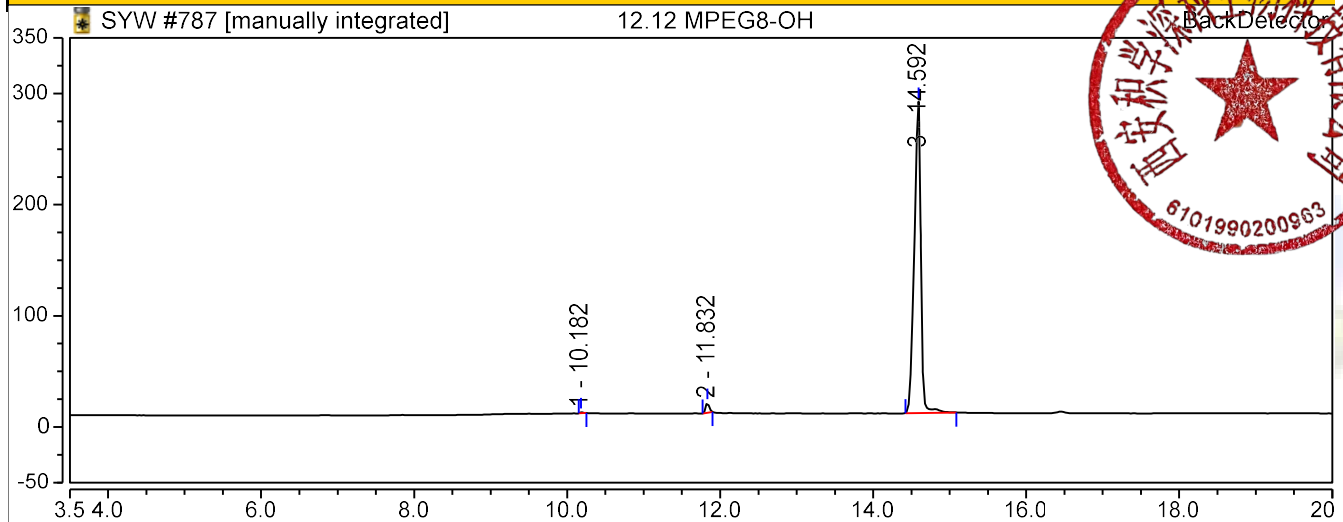

No.	Peak Name	Retention Time min	Area pA*min	Height pA	Relative Area %	Relative Height %
1		10.182	0.049	1	0.17	0.37
2		11.832	0.484	9	1.69	3.07
3		14.592	28.039	280	98.14	96.56
Total:			29	290	100.00	100.00