


Peak Analysis

Injection Details					
Injection Name:	m-3-sh-??			Run Time (min):	10.67
Vial Number:	82			Injection Volume:	5.00
Injection Type:	Unknown				
Calibration Level:					
Instrument Method:	80 hold 2 min 30 per 280 hold 2 min				
Processing Method:	Qualitative			Dilution Factor:	1.0000
Injection Date/Time:	20/Sep/23 16:38			Sample Weight:	1.0000

Chromatogram

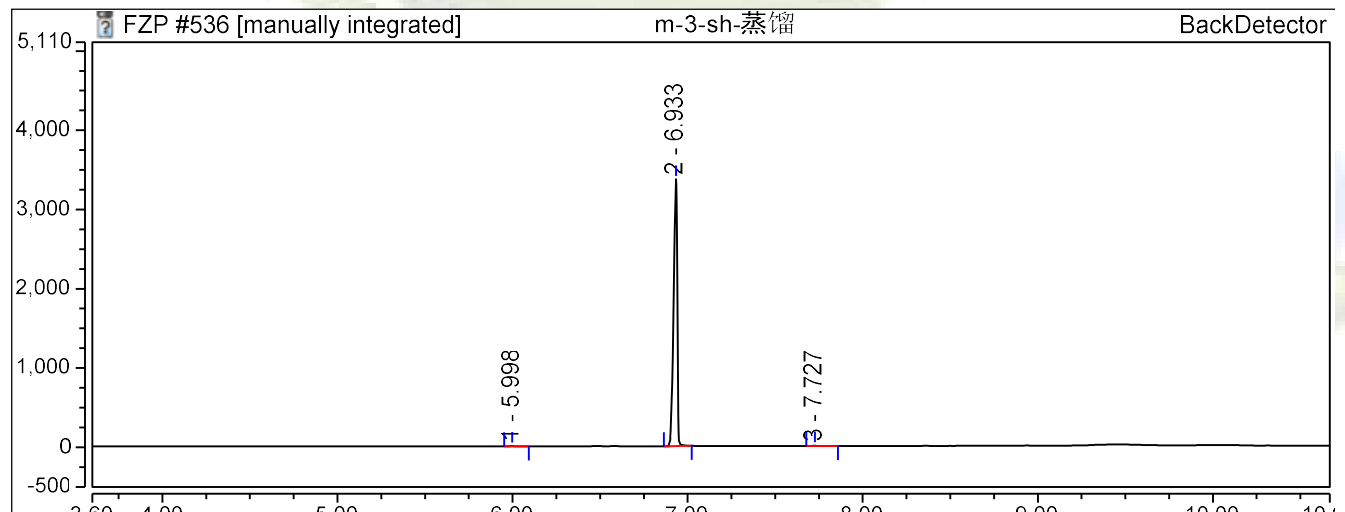

No.	Peak Name	Retention Time min	Area pA*min	Height pA	Relative Area %	Relative Height %
1		5.998	0.065	2	0.08	0.07
2		6.933	79.897	3,367	99.83	99.85
3		7.727	0.069	3	0.09	0.08
Total:			80	3,372	100.00	100.00

Mass Spectrum

Spectral plot could not be created.
No spectra selected.