


## Chromatogram and Results

Injection Details			
Injection Name:	M-P6-NH2-0806	Run Time (min):	11.50
Vial Number:	21	Injection Volume:	1.00
Injection Type:	Unknown	Channel:	BackDetector
Calibration Level:		Wavelength:	n.a.
Instrument Method:	80 hold 2 min 30 per 310 hold 2 min	Bandwidth:	n.a.
Processing Method:	Basic Quantitative(3)	Dilution Factor:	1.0000
Injection Date/Time:	06/Aug/24 23:00	Sample Weight:	1.0000

### Chromatogram

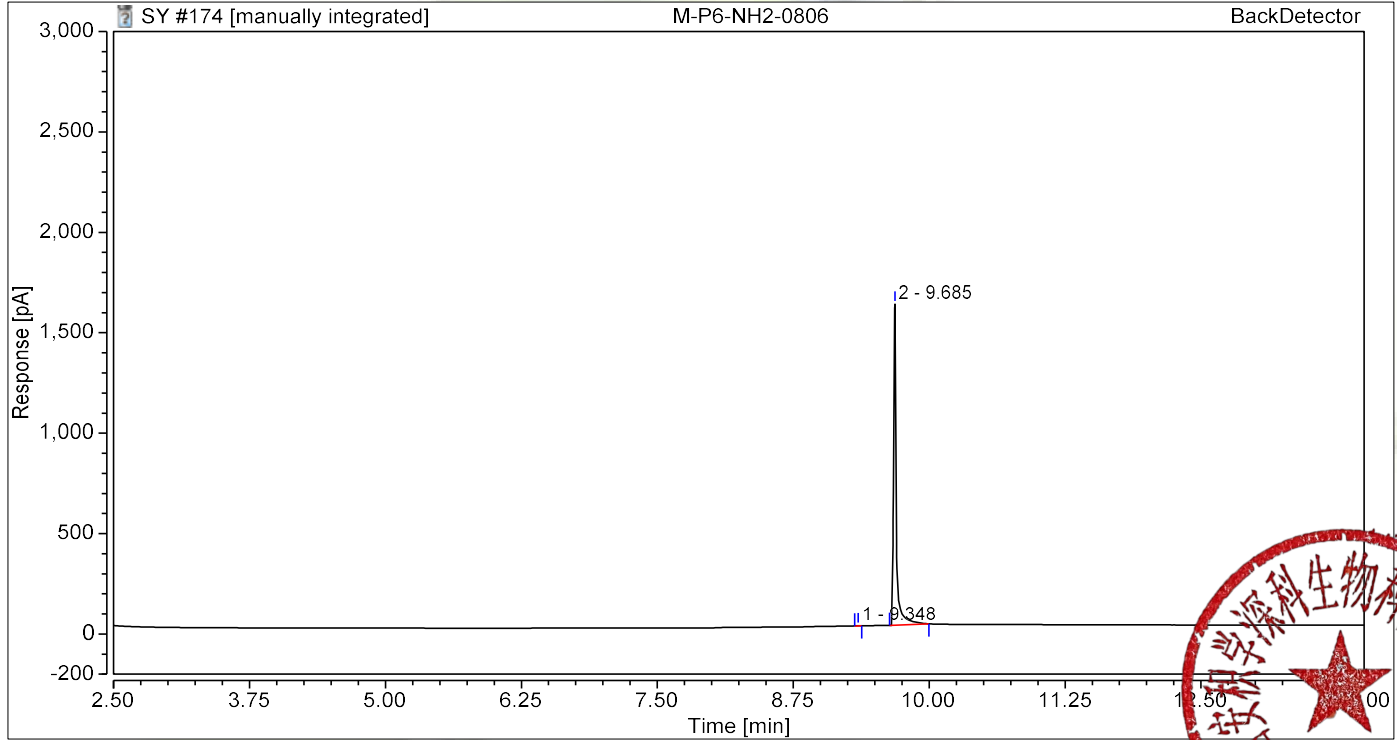

Integration Results							
No.	Peak Name	Retention Time min	Area pA*min	Height pA	Relative Area %	Relative Height %	Amount ng
1		9.348	0.011	0.324	0.02	0.02	n.a.
2		9.685	48.373	1598.241	99.98	99.98	n.a.
Total:			48.384	1598.565	100.00	100.00	

