


## Chromatogram and Results

Injection Details			
Injection Name:	tBu-PEG2-OH-240828	Run Time (min):	12.50
Vial Number:	13	Injection Volume:	1.00
Injection Type:	Unknown	Channel:	BackDetector
Calibration Level:		Wavelength:	n.a.
Instrument Method:	80 hold 2 min 20 per 280 hold 2 min - Copy	Bandwidth:	n.a.
Processing Method:	Basic Quantitative(3)	Dilution Factor:	1.0000
Injection Date/Time:	28/Aug/24 17:16	Sample Weight:	1.0000

### Chromatogram

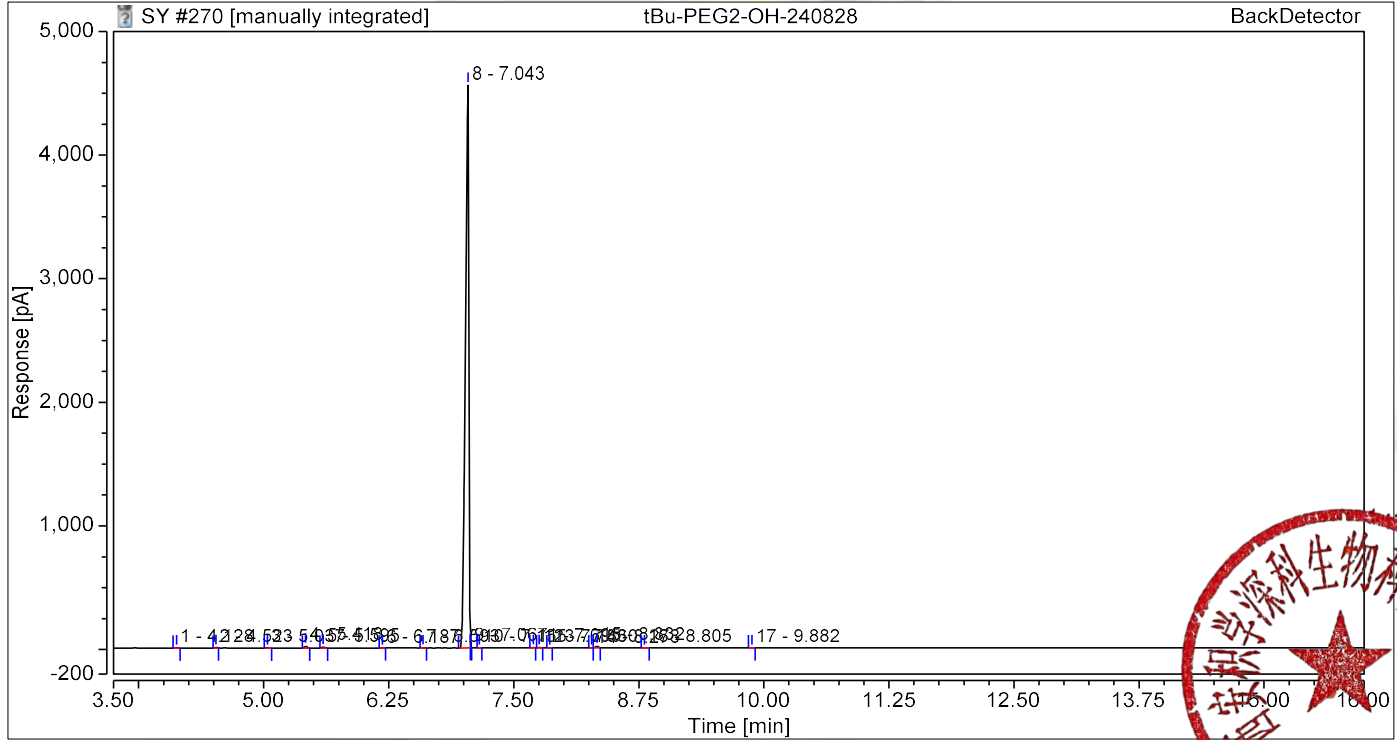

### Integration Results

No.	Peak Name	Retention Time min	Area pA*min	Height pA	Relative Area %	Relative Height %	Area
1		4.128	0.035	1.412	0.02	0.03	n.a.
2		4.523	0.078	3.371	0.04	0.07	n.a.
3		5.037	0.035	1.541	0.02	0.03	n.a.
4		5.418	0.420	17.666	0.23	0.38	n.a.
5		5.595	0.251	7.761	0.14	0.17	n.a.
6		6.187	0.017	0.498	0.01	0.01	n.a.
7		6.593	0.063	2.711	0.04	0.06	n.a.
8		7.043	178.240	4552.591	99.09	98.36	n.a.
9		7.067	0.038	11.547	0.02	0.25	n.a.
10		7.155	0.016	1.060	0.01	0.02	n.a.
11		7.695	0.079	3.408	0.04	0.07	n.a.
12		7.753	0.075	3.204	0.04	0.07	n.a.
13		7.860	0.029	1.215	0.02	0.03	n.a.
14		8.278	0.010	0.502	0.01	0.01	n.a.
15		8.332	0.424	17.177	0.24	0.37	n.a.
16		8.805	0.029	0.985	0.02	0.02	n.a.
17		9.882	0.043	1.683	0.02	0.04	n.a.
Total:			179.882	4628.334	100.00	100.00	