


## Chromatogram and Results

Injection Details			
Injection Name:	tBu-PEG3-OH-240828	Run Time (min):	12.50
Vial Number:	139	Injection Volume:	1.00
Injection Type:	Unknown	Channel:	BackDetector
Calibration Level:		Wavelength:	n.a.
Instrument Method:	80 hold 2 min 20 per 280 hold 2 min - Copy	Bandwidth:	n.a.
Processing Method:	Basic Quantitative(3)	Dilution Factor:	1.0000
Injection Date/Time:	28/Aug/24 11:14	Sample Weight:	1.0000

### Chromatogram

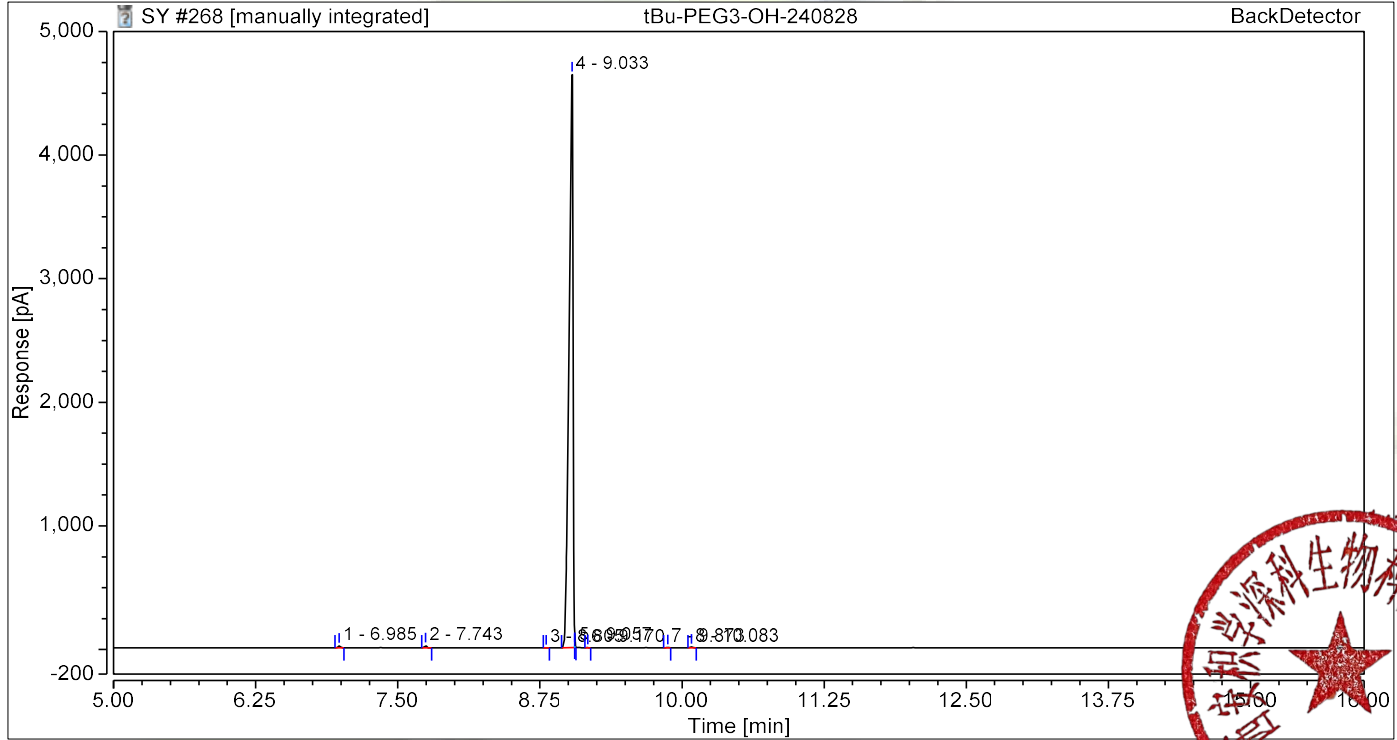

### Integration Results

No.	Peak Name	Retention Time min	Area pA*min	Height pA	Relative Area %	Relative Height %	Area
1		6.985	0.392	16.709	0.21	0.36	n.a.
2		7.743	0.407	18.143	0.21	0.39	n.a.
3		8.805	0.014	0.490	0.01	0.01	n.a.
4		9.033	188.407	4634.878	99.39	98.64	n.a.
5		9.057	0.064	17.438	0.03	0.37	n.a.
6		9.170	0.028	1.211	0.01	0.03	n.a.
7		9.873	0.075	3.074	0.04	0.07	n.a.
8		10.083	0.180	6.899	0.09	0.15	n.a.
Total:			189.567	4698.842	100.00	100.00	